

Carbon Dioxide Optical Sensors Using Near- and Mid-Infrared Semiconductor Lasers

CLÉMENT JACQUEMIN^{1,2,*}, FLORENT DEFOSSEZ¹, RAPHAËL VALLON¹, BERTRAND PARVITTE¹, GRÉGOR Y MAISON², MATHIEU CARRAS², AND VIRGINIE ZENINARI¹

¹ Université de Reims Champagne Ardenne, Centre National de la Recherche Scientifique, Groupe de Spectrométrie Moléculaire et Atmosphérique, UMR 7331, 51097 Reims, France

² MirSense, 1 Rue Jean Rostand, Campus Eiffel, 91400 Orsay, France

*clement.jacquemin1@etudiant.univ-reims.fr

Tunable Laser Absorption Spectroscopy

Laser
→ High-brightness and purely monochromatic light source

Tunable
→ Allows to precisely describe the absorption shape of the sample by scanning the laser wavelength

- Absorption shape**
- + Associated wavelength
 - = Specific to a single chemical species
-
- + Intensity of the absorption
- = Quantification


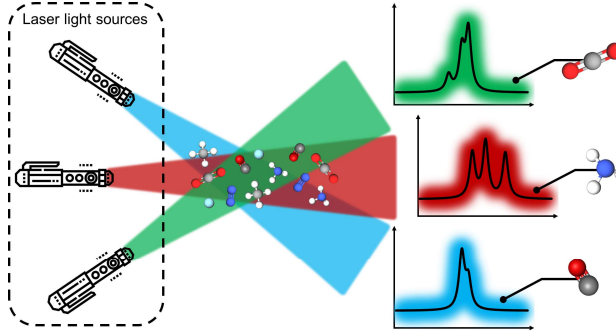



Illustration of the TLAS principle. Each color correspond to a distinct wavelength. Depending on the wavelength used, the observed absorption will not be the same, as represented by the projected-shadow like plot on the right. This allows to distinguish precisely the different chemical compounds.

Algorithm that match the acquired spectrum with known absorption pattern

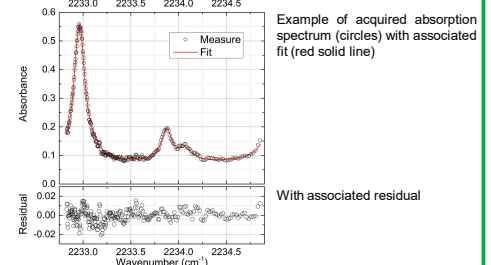


Absorption shape only rely on the chemical species
Intensity only rely on molecular concentration and interaction length → **Calibration free method**

Carbon Dioxide Optical Sensors

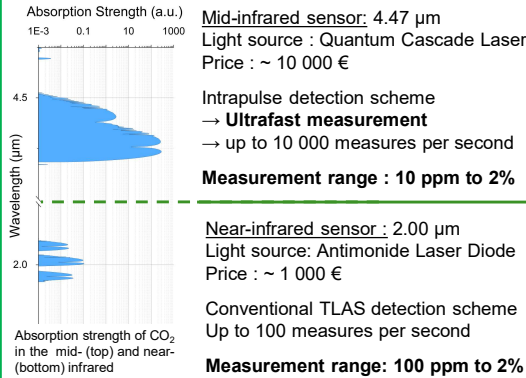

This type of sensor can be used to detect any chemical species with absorption features in the infrared. For example, the lowest detectable absorption of CO₂ with the mid-infrared sensor is equivalent to an absorption of 3 ppb of NO₂. It is just necessary to use a laser source with a wavelength that matches the absorption of the target molecule.

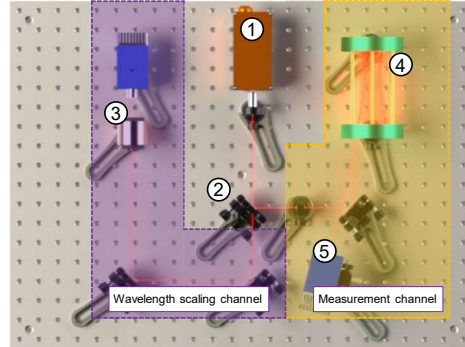


3D top view of a typical experimental setup
1: Laser source 3: Fabry-Pérot etalon 5: Infrared detector
2: Beam splitter 4: Sampling cell

Sampling Cell: Dense Pattern Multipass Cell

Air flow between two mirrors (distance = 15 cm)

Light makes multiple reflections in the cell : Up to 200 pass
→ Increase the effective path length
→ **15 cm base-length × 200 pass = 30 m**

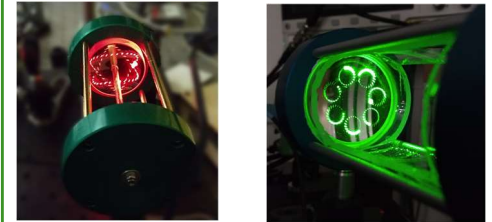

Multipass cell with visible alignment laser. (Left: cell used with quantum cascade laser | Right: cell used with laser diode)

Outdoor campaign

Deployed on field: invitation to a gas release trial at CENZUB
→ Centre d'entrainement aux actions en zone urbaine (Military training area, France)

Managed by the INERIS

Trial :

→ Several successive massive releases of CO₂ in a fake city with different kind of buildings


→ Various sensor technologies located at different spots to study the gas dispersion



Top view photo of trial site. The numbered red pins indicate the positions of the sensors during the successive trial



Picture of the gas source during a release

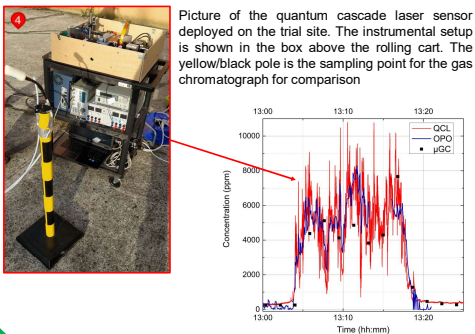


Comparison with reference instrument : NDIR Sensor & Gas Chromatograph

→ Good agreement with other measurement systems

- **Higher measurement range**
- **Higher acquisition rate**
- **Higher temporal resolution**
- Allows the study of high-speed phenomena

Fully qualified sensors to be deployed

Picture of the laser diode sensor deployed on the trial site. The instrumental setup is enclosed in the box above the rolling cart. The device above the box is an NDIR sensor (ULCO, Dunkerque) for comparison

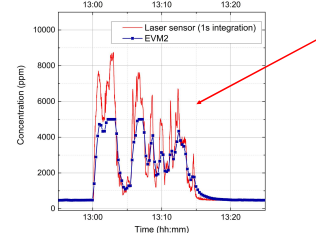

Perspectives

- Improve the detection limits (For leak detection application)
- Lighter and more compact device: Sampling volume down to tens cm³ (Under development)
- Develop a dedicated driving and acquisition electronics
- **Application on other gases:** N₂O, CH₄, NO₂, ... (Greenhouse gases, Pollutants)

Acknowledgments :

The authors thank INERIS (Institut National de l'Environnement Industriel et des Risques) and Commandant Faget for the invitation to the trial. The authors also thank the ANR Ethylas project for funding the multipass cell used in this work and mirSense for funding the PhD of Clément Jacquemin by a CIFRE contract and providing the laser source.

The work on the QCL sensor has been published in a scientific journal. Scan the QR code to access to the journal page.

